


# 0.924+/- 0.002 X-Band Phase Shifter QC Batch 4 (Scrapped)



# 0.970 $\pm$ 0.002 X-Band Phase Shifter QC Batch 4 (Scrapped)

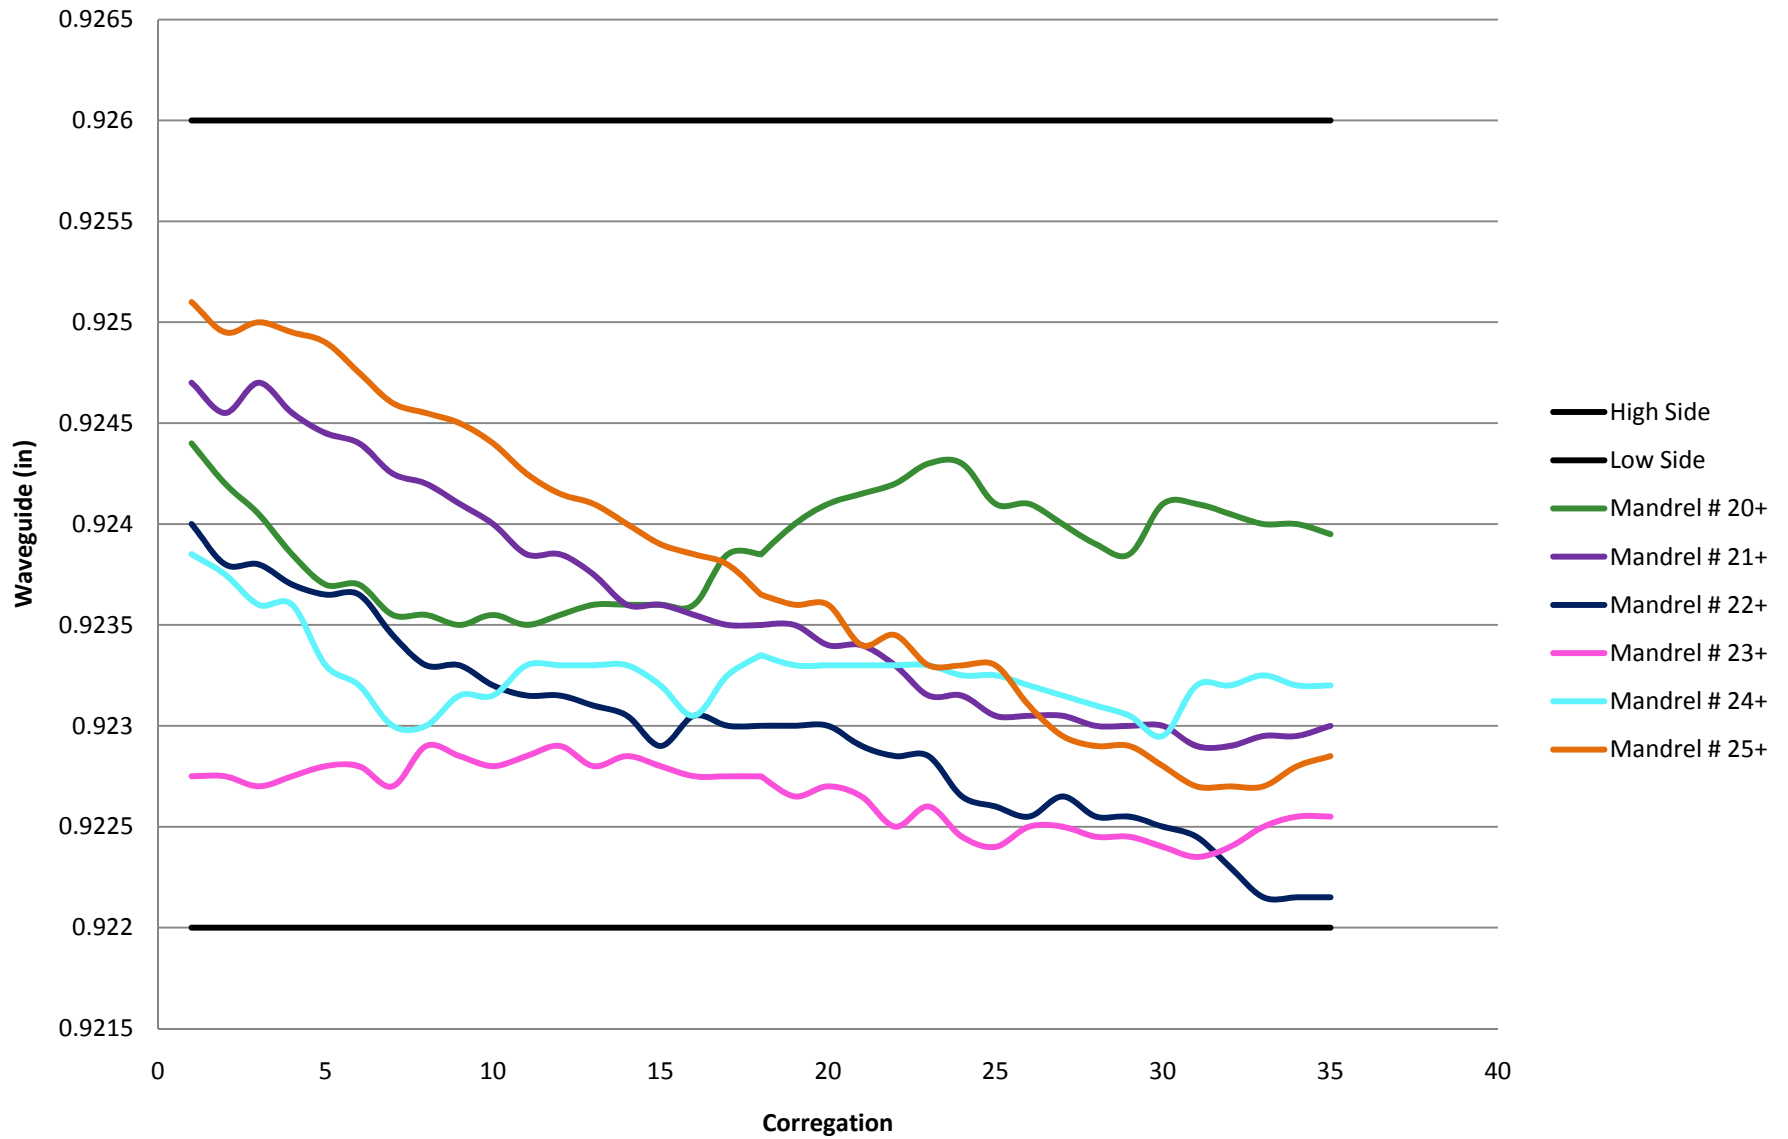