


# 0.924 $\pm$ 0.002 X-Band Phase Shifter QC Batch 5 (Re-Runs)



# 0.970 $\pm$ 0.002 X-Band Phase Shifter QC Batch 5 (Re-Run)

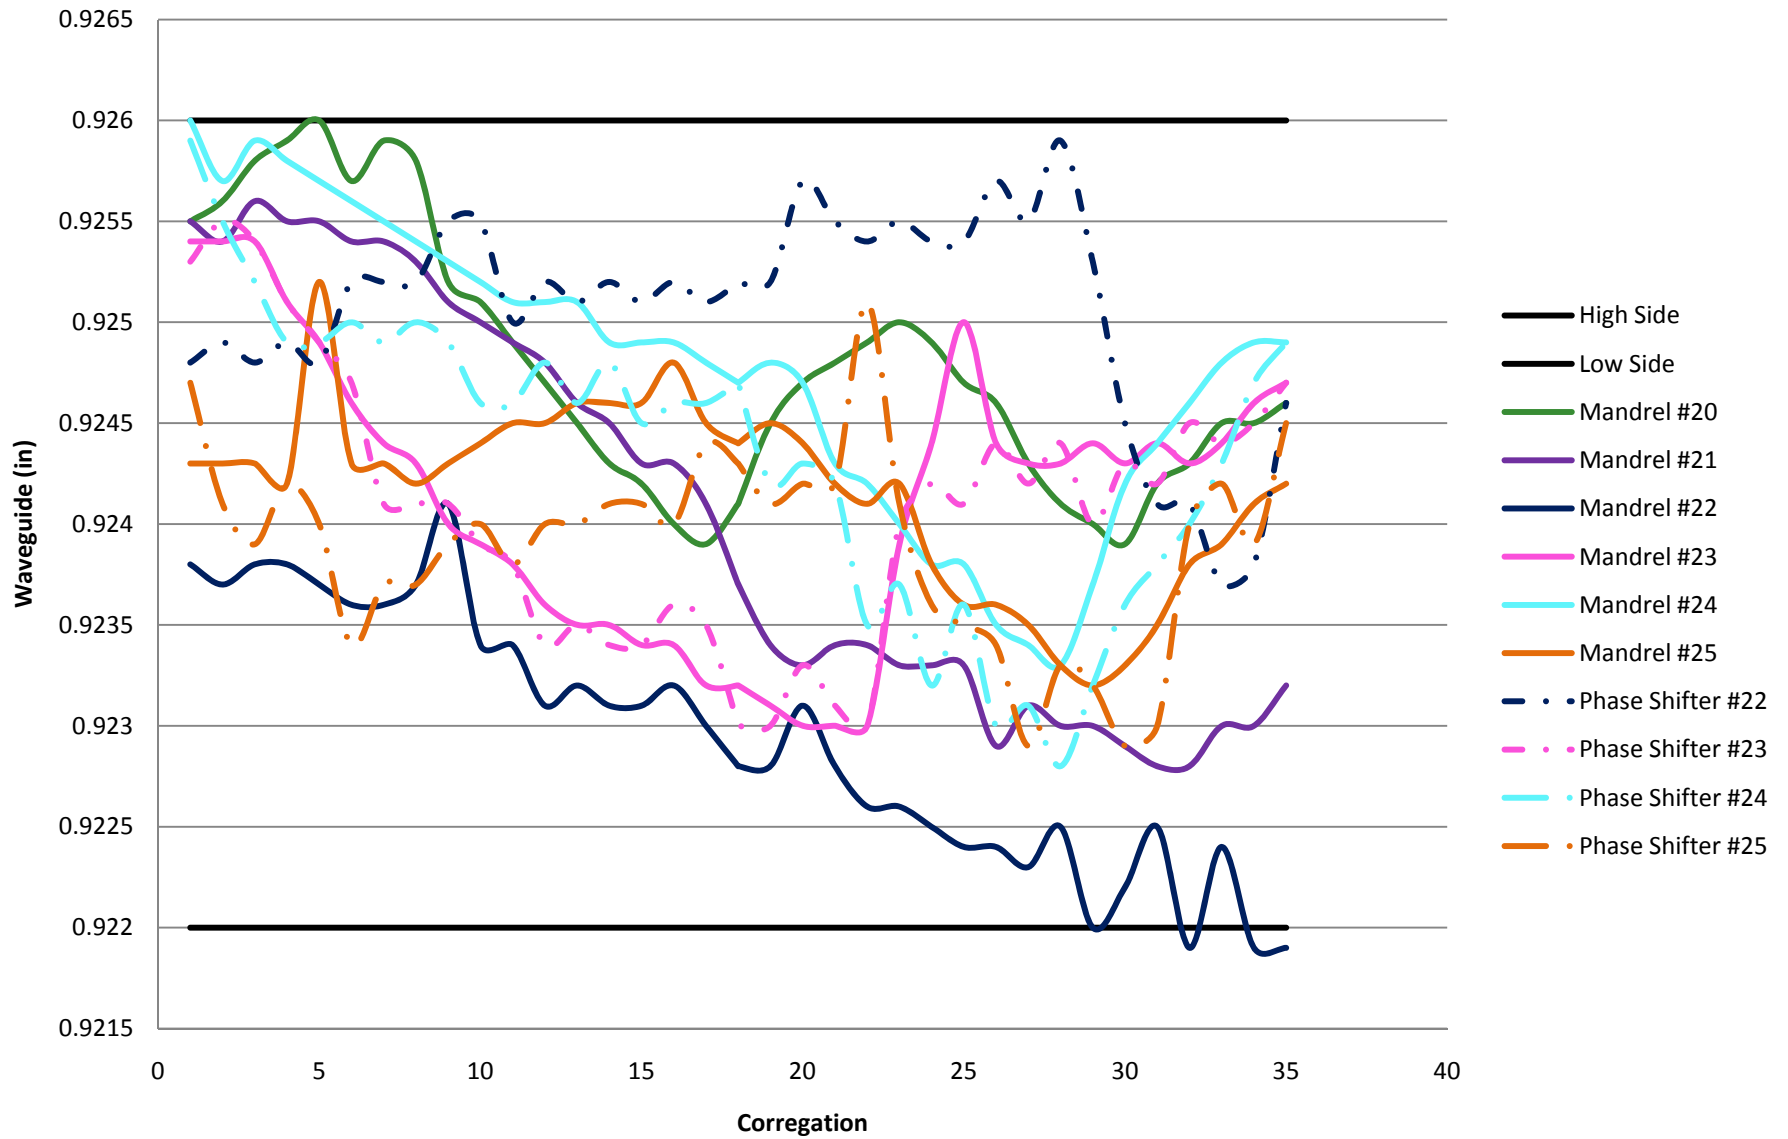